



Scottsdale Crime Lab

VENDOR CONTROL INSERTS  
FOR BLOOD SAMPLES  
ANALYZED:

April 10, 2012---July 28, 2012

Please make copies only, do not remove or mix these items  
with other time periods.



## Certificate of Analysis

### Ethanol 0.400 Calibrator

Solution Lot	091610-4
Preparation Date	09/16/10
Prepared By	RFB B1463
Method	Gravimetric
Solvent	UltraPure Water
Amount	500 ml
Storage	Working container: room temp Stock solution: refrigerate
Expiration Date	09/2013
Analysis Method	GC/FID
Calibration Curve	Linear Regression
Number of Points	4
Date Analyzed	09/30/10
Linearity	0.9999
Calibrators	Cerilliant <sup>1</sup>
Measured Value	0.399 <sup>2</sup>
Difference from target	0.001
Verified	RFB B1463

<sup>1</sup> 0.4, 0.2, 0.1, and 0.02 calibrators, respectively: Cerilliant FN040909-01, Cerilliant FN070209-01, Cerilliant FN 102609-03, and Cerilliant FN 030409-01

<sup>2</sup> Average of 4 measurements




## Certificate of Analysis

### Ethanol 0.200 Calibrator

Solution Lot	091610-2
Preparation Date	09/16/10
Prepared By	RFB B1463
Method	Gravimetric
Solvent	UltraPure Water
Amount	500 ml
Storage	Working container: room temp Stock solution: refrigerate
Expiration Date	09/2013
Analysis Method	GC/FID
Calibration Curve	Linear Regression
Number of Points	4
Date Analyzed	09/30/10
Linearity	0.9999
Calibrators	Cerilliant <sup>1</sup>
Measured Value	0.199 <sup>2</sup>
Difference from target	0.001
Verified	RFB B1463

<sup>1</sup> 0.4, 0.2, 0.1, and 0.02 calibrators, respectively: Cerilliant FN040909-01, Cerilliant FN070209-01, Cerilliant FN 102609-03, and Cerilliant FN 030409-01

<sup>2</sup> Average of 4 measurements



## Certificate of Analysis

### Ethanol 0.100 Calibrator

Solution Lot	091610-1
Preparation Date	09/16/10
Prepared By	RFB B1463
Method	Gravimetric
Solvent	UltraPure Water
Amount	500 ml
Storage	Working container: room temp Stock solution: refrigerate
Expiration Date	09/2013
Analysis Method	GC/FID
Calibration Curve	Linear Regression
Number of Points	4
Date Analyzed	09/30/10
Linearity	0.9999
Calibrators	Cerilliant <sup>1</sup>
Measured Value	0.099 <sup>2</sup>
Difference from target	0.001

Verified	RFB B1463
----------	-----------

---

<sup>1</sup> 0.4, 0.2, 0.1, and 0.02 calibrators, respectively: Cerilliant FN040909-01, Cerilliant FN070209-01, Cerilliant FN 102609-03, and Cerilliant FN 030409-01

<sup>2</sup> Average of 4 measurements



## Certificate of Analysis

### Ethanol 0.020 Calibrator

Solution Lot	091610-02
Preparation Date	09/16/10
Prepared By	RFB B1463
Method	Gravimetric
Solvent	UltraPure Water
Amount	500 ml
Storage	Working container: room temp Stock solution: refrigerate
Expiration Date	09/2013
Analysis Method	GC/FID
Calibration Curve	Linear Regression
Number of Points	4
Date Analyzed	09/30/10
Linearity	0.9999
Calibrators	Cerilliant <sup>1</sup>
Measured Value	0.021 <sup>2</sup>
Difference from target	0.001
Verified	RFB B1463

<sup>1</sup> 0.4, 0.2, 0.1, and 0.02 calibrators, respectively: Cerilliant FN040909-01, Cerilliant FN070209-01, Cerilliant FN 102609-03, and Cerilliant FN 030409-01

<sup>2</sup> Average of 4 measurements



# Whole Blood Ethanol Control Level 2

## INTENDED USE

### FOR IN VITRO DIAGNOSTIC USE

LiquiSP<sup>TM</sup> Whole Blood Ethanol Control is an assayed quality control material intended for use in monitoring the accuracy and precision of the quantitative determination of ethanol in whole blood.

## SUMMARY AND PRINCIPLE

This product is to be used exactly as directed for the patient sample in order to monitor, and thus minimize the potential for technical and performance errors in routine testing.

## PRODUCT DESCRIPTION

LiquiSP<sub>x</sub> Whole Blood Ethanol Control is prepared from stabilized normal human whole blood with the addition of ethanol. This product has been assigned lot-specific ethanol values using quantitative analytical methods. This product is packaged 5.0 mL per vial.

## STORAGE AND STABILITY

LiquiSP<sub>x</sub> Whole Blood Ethanol Control is stable until the expiration date on the package when stored unopened at ≤ -20°C and 30 days after opening when stored at 2-8°C. Once thawed and unopened, the product is stable for 12 months at 2-8°C. This product may be thawed and re-frozen one time only. Discard any contaminated material. Microbial contamination is evidenced by an increase in turbidity and/or a characteristic odor.

## PRECAUTIONS

### Human source material. Treat as potentially infectious.

Each serum/plasma donor unit used in the manufacture of this product has been tested by FDA accepted methods and found non-reactive for the presence of HBsAg and antibody to HIV-1/2, HCV and HIV-1 Ag. While these methods are highly accurate, they do not guarantee that all infected units will be detected. Because no known test method can offer complete assurance the hepatitis B virus, hepatitis C virus, human immunodeficiency virus (HIV) or other infectious agents are absent, all products containing human source material should be considered potentially infectious and handled with the same precautions used with patient specimens.

This product contains 0.09% sodium azide as a preservative. Sodium azide may react with lead and copper plumbing to form potentially explosive compounds. Flush with excess water upon disposal.

## PROCEDURE

Allow the refrigerated controls to warm to room temperature (18-25° C) and gently swirl the control material prior to use in order to ensure product homogeneity. QC materials should be used in accordance with local, state, and/or federal regulations or accreditation requirements.

## LIMITATIONS

This material is a control for methods listed in the ASSIGNED VALUES section; it is not to be used as a calibrator. Accurate and reproducible results are dependent upon properly functioning instruments, reagents, standardization, and proper laboratory techniques. Individual laboratories may not obtain the mean assigned value as listed.

## VALUE ASSIGNMENT

The mean values and expected ranges printed in this insert were derived from extensive replicate analyses and are specific for this lot.

Values listed below were generated by Cliniqua, the reagent/instrument manufacturer and/or independent laboratories in accordance with an established protocol.

Procedural or assay modifications may alter the mean value obtained. Each laboratory should establish its own parameters of precision; use the mean assigned values and expected ranges provided only as guidelines.

## ASSIGNED VALUES

Level 2		Lot No.: 1002171 Exp. Date: 2014-03	
Method	Units	Mean	Expected Range
Gas Chromatography	mg/dL	194	175 - 214

## REFERENCES

Baselt, R.C. Analytical Procedures for Therapeutic Drug Monitoring and Emergency Toxicology. Littleton, MA, PSG Publishing, 1987.



For in vitro diagnostic use



See package insert for proper use

## CLINIQA CORPORATION

288 Distribution St.  
San Marcos, CA 92078  
USA

## SALES AND TECHNICAL SUPPORT

P: 800 728 5205  
+1 760 744 1900  
F: +1 760 571 5198  
[www.cliniqua.com](http://www.cliniqua.com)

## FOR ORDERS AND CUSTOMER SERVICE

P: 800 728 5205  
+1 760 744 1900  
F: +1 760 571 5197  
[csgroup@cliniqua.com](mailto:csgroup@cliniqua.com)



CEpartner4U  
Esdoornlaan 13  
3951 DB Maarn, The Netherlands  
P: +31 (0)6 516 536 26

## RE-ORDER INFORMATION Whole Blood Ethanol Control

Catalog No.



93211

Level 1, 6 x 5 mL

Catalog No.



93212

Level 2, 6 x 5 mL

Catalog No.



93213

Level 3, 6 x 5 mL





CE

# Whole Blood Ethanol Control Level 2

## INTENDED USE FOR IN VITRO DIAGNOSTIC USE

LiquiSP<sup>TM</sup> Whole Blood Ethanol Control is an assayed quality control material intended for use in monitoring the accuracy and precision of the quantitative determination of ethanol in whole blood.

## SUMMARY AND PRINCIPLE

This product is to be used exactly as directed for the patient sample in order to monitor, and thus minimize the potential for technical and performance errors in routine testing.

## PRODUCT DESCRIPTION

LiquiSP<sub>x</sub> Whole Blood Ethanol Control is prepared from stabilized normal human whole blood with the addition of ethanol. This product has been assigned lot-specific ethanol values using quantitative analytical methods. This product is packaged 5.0 mL per vial.

## STORAGE AND STABILITY

LiquiSP<sub>x</sub> Whole Blood Ethanol Control is stable until the expiration date on the package when stored unopened at 2-8°C and 45 days after opening when stored at 2-8°C. Discard any contaminated material. Microbial contamination is evidenced by an increase in turbidity and/or a characteristic odor.

## PRECAUTIONS

**Human source material. Treat as potentially infectious.**

Each serum/plasma donor unit used in the manufacture of this product has been tested by FDA accepted methods and found non-reactive for the presence of HBsAg and antibody to HIV-1/2, HCV and HIV-1 Ag. While these methods are highly accurate, they do not guarantee that all infected units will be detected. Because no known test method can offer complete assurance the hepatitis B virus, hepatitis C virus, human immunodeficiency virus (HIV) or other infectious agents are absent, all products containing human source material should be considered potentially infectious and handled with the same precautions used with patient specimens.

This product contains 0.09% sodium azide as a preservative. Sodium azide may react with lead and copper plumbing to form potentially explosive compounds. Flush with excess water upon disposal.

## PROCEDURE

Allow the refrigerated controls to warm to room temperature (18-25°C) and gently swirl the control material prior to use in order to ensure product homogeneity. QC materials should be used in accordance with local, state, and/or federal regulations or accreditation requirements.

## LIMITATIONS

This material is a control for methods listed in the ASSIGNED VALUES section; it is not to be used as a calibrator. Accurate and reproducible results are dependent upon properly functioning instruments, reagents, standardization, and proper laboratory techniques. Individual laboratories may not obtain the mean assigned value as listed.

## VALUE ASSIGNMENT

The mean values and expected ranges printed in this insert were derived from extensive replicate analyses and are specific for this lot.

Values listed below were generated by Cliniqua, the reagent/instrument manufacturer and/or independent laboratories in accordance with an established protocol.

Procedural or assay modifications may alter the mean value obtained. Each laboratory should establish its own parameters of precision; use the mean assigned values and expected ranges provided only as guidelines.

## ASSIGNED VALUES

Level 2		Lot No.: 1002171A Exp. Date: 2014-03	
Method	Units	Mean	Expected Range
Gas Chromatography	mg/dL	194	175 - 214

## REFERENCES

Baselt, R.C. Analytical Procedures for Therapeutic Drug Monitoring and Emergency Toxicology. Littleton, MA, PSG Publishing, 1987.



For in vitro diagnostic use



See package insert for proper use



### CLINIQA CORPORATION

288 Distribution St.  
San Marcos, CA 92078  
USA

### SALES AND TECHNICAL SUPPORT

P: 800 728 5205  
+1 760 744 1900  
F: +1 760 571 5198

[www.cliniqua.com](http://www.cliniqua.com)

### FOR ORDERS AND CUSTOMER SERVICE

P: 800 728 5205  
+1 760 744 1900  
F: +1 760 571 5197

[csgroup@cliniqua.com](mailto:csgroup@cliniqua.com)



CEpartner4U  
Esdorplan 13  
3951 DB Maarn, The Netherlands  
P: +31 (0)6 516 536 26

## RE-ORDER INFORMATION Whole Blood Ethanol Control

Catalog No.

**REF** 93211

Level 1, 6 x 5 mL

Catalog No.

**REF** 93212

Level 2, 6 x 5 mL

Catalog No.

**REF** 93213

Level 3, 6 x 5 mL





*Certificate of Analysis*  
*Certified Reference Standard - NIST Traceable*

**Ethanol-10**  
*Ethyl Alcohol*

ISO GUIDE 34  
 ACCREDITED  
 CERTIFICATE ARI1353  
 ISO/IEC 17025  
 ACCREDITED  
 CERTIFICATE ARI1352  
 ISO 9001:2000  
 CERTIFIED  
 CERTIFICATE 3854

Catalog Number: E-040  
 Solution Lot: FN061108-01  
 Expiration Date: June 2013  
 Diluent: Water  
 Volume per Ampule: 1.2 mL  
 Storage: Protect from light, refrigerate. Do not freeze.  
 Intended Use: For laboratory use only. Not suitable for human or animal consumption.

- Expiration Date has been established through real time stability studies
- Ampules are overfilled to ensure a minimum 1.2 mL volume fill. We advise laboratories to use measured volumes of this standard solution when dilution or exact volume is required.

Component	Chromatographic Purity	Concentration
Ethanol	100%	10.00 ± 0.04 mg/dL
<ul style="list-style-type: none"> <li>Uncertainty of the concentration is expressed as an expanded uncertainty in accordance with ISO 17025 and ISO Guide 34 at the 95% confidence interval using a coverage factor of k=2, has been calculated by statistical analysis of our production system and incorporates uncertainty of the purity factor, material density and mass.</li> </ul>		

**NIST Traceability:**

- This calibration was conducted using standards whose values are traceable to the SI through NIST.
- Gravimetrically prepared using qualified balances calibrated semi-annually by Mettler Toledo using NIST traceable weights. Calibration verification is performed weekly and prior to each use utilizing NIST traceable weights. Each balance has been assigned a minimum weighing by Mettler Toledo taking into consideration the balance and installed environmental conditions to ensure weighing complies with USP tolerances of no more than 0.1% relative error.
- Concentration is verified against a 4-point calibration curve prepared from a NIST SRM.

**Solution Standard Analysis and Homogeneity:**

Solution Standard	Lot Number	Concentration compared Calibration Curve (mg/mL)		Homogeneity %RSD	
		Actual Results	Acceptance Criteria	Actual Results	Acceptance Criteria
		<u>NIST SRM Lot # 2897</u>			
New Lot	FN061108-01	10.15	± 2.0%	0.7%	≤ 2.0%
Prior Lot	FN011107-01	10.15	± 2.0%	0.3%	≤ 2.0%
<ul style="list-style-type: none"> <li>Concentration is calculated as the average of multiple analyses compared to a calibration curve prepared from a NIST SRM.</li> <li>Homogeneity of the New Lot is ensured through rigorous production process controls developed through statistical analysis and risk assessment of each process and verified by analysis of the solution standard. The %RSD of samples pulled from across the lot demonstrates homogeneity of the New Lot.</li> <li>The %RSD of the Prior Lot represents variability of the analysis.</li> </ul>					

Cerilliant certifies that this standard meets the specifications stated in this certificate and warrants this product to meet the stated acceptance criteria through the expiration date.



*Lara Sparks*  
 Lara Sparks, Quality Assurance Director

*February 14, 2009*  
 Date



### Solution Standard Assay Parameters

Analysis Method: GC/FID Headspace  
 Column: DB-ALC1 30 m x 0.53 mm ID, 3.0 µm film thickness  
 Temp Program: 40°C hold for 12 min  
 Injector Temp: 200°C  
 Detector Temp: 250°C


### NIST Calibration Curve

NIST SRM Lot # 2897  
 Calibration Curve: Linear Regression  
 Number of Points 4  
 Linearity (r): 1.000

*Each point is analyzed in triplicate*

### Neat Material Verification

GC/FID Headspace Analysis

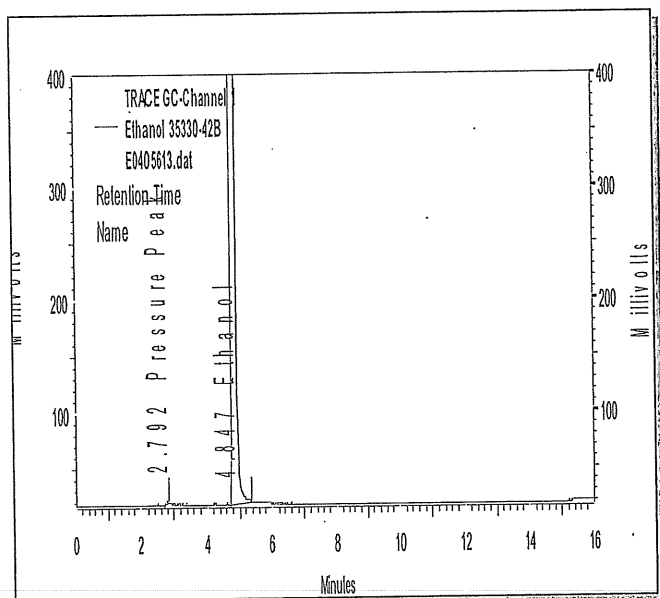

### COA Revision History

Revision	Date	Reason for Revision
00	8/4/2008	Initial version
01	2/18/2009	Revised COA template to comply with ISO/IEC 17025 requirements.




# Certificate of Analysis

## Certified Reference Material - NIST Traceable

### Ethanol-20

Ethyl Alcohol



Catalog Number: E-056  
Solution Lot: FN030409-01  
Expiration Date: March 2014  
Diluent: Water  
Volume per Ampule: 1.2 mL  
Storage: Protect from light, refrigerate. Do not freeze.  
Intended Use: For laboratory use only. Not suitable for human or animal consumption.

- Expiration Date has been established through real time stability studies.
- Ampules are overfilled to ensure a minimum 1.2 mL volume fill. We advise laboratories to use measured volumes of this solution standard before diluting to the desired concentration.

Component	Chromatographic Purity	Concentration
Ethanol	100%	20.00 ± 0.07 mg/dL

Chromatographic purity of the solution is verified post ampuling to provide assurance of no contamination or degradation during manufacturing.

Uncertainty of the concentration is expressed as an expanded uncertainty in accordance with ISO/IEC 17025 and ISO Guide 34 at the 95% confidence interval using a coverage factor of k=2 and has been calculated by statistical analysis of our production system. Uncertainty includes uncertainty of the purity factor, material density and mass. Purity factor uncertainty incorporates uncertainty of all analyses performed to characterize the raw material including chromatographic purity and residual water. Mass uncertainty incorporates uncertainty of the balance in its installed environment and weighing technique and was determined through repeatability experiments using Cerilliant established weighing procedures.

This standard meets the definition of a Certified Reference Material in accordance with ISO Guide 34.

### Traceability

- This standard and its preparation are fully traceable to the SI through NIST.
- This standard was gravimetrically prepared using qualified balances calibrated semi-annually by Mettler Toledo, an ISO/IEC 17025 accredited company, using NIST traceable weights. Calibration verification is performed weekly through the range of the balance and then prior to each use. All calibration verifications are performed utilizing NIST traceable weights which are externally calibrated on an annual basis by a qualified ISO 17025 accredited calibration laboratory. Weight tapes verifying pre-use balance calibration are included in the production batch record for this standard. Each balance has been assigned a minimum weighing by Mettler Toledo taking into consideration the balance and installed environmental conditions to ensure weighing complies with USP tolerances of no more than 0.1% relative error.
- Concentration is analytically verified by multiple analyses directly to a NIST SRM.

Cerilliant certifies that this standard meets the specifications stated in this certificate and warrants this product to meet the stated acceptance criteria through the expiration date when stored unopened as recommended. Product should be used shortly after opening to avoid concentration changes due to evaporation. Warranty does not apply to ampoules stored after opening.



*Lara Sparks*  
Lara Sparks, Quality Assurance Director

April 27, 2009  
Date

# Certificate of Analysis


ISO GUIDE 34  
ACCREDITED  
CERTIFICATE AR1353

ISO/IEC 17025  
ACCREDITED  
CERTIFICATE AT1262

ISO 9001:2000  
CERTIFIED  
CERTIFICATE 3052

## Ethanol-150

*Ethyl alcohol*

<b>Catalog Number:</b>	E-041	
<b>Solution Lot:</b>	FN020108-01	
<b>Expiration Date:</b>	February 2013	
<b>Solvent:</b>	Water	
<b>Amount per Ampule:</b>	1.2 mL	
<b>Storage:</b>	Protect from light, refrigerate. Do not freeze.	
<b>Handling:</b>	We advise laboratories to use measured volumes of this standard solution before diluting to the desired concentration.	
<b>Intended Use:</b>	For laboratory use only. Not suitable for human or animal consumption.	

Component	Chromatographic Purity <sup>1</sup>	Concentration <sup>2</sup>
Ethanol	99%	150.0 ± 4.7 mg/dL

<sup>1</sup> See following pages for more information.

<sup>2</sup> The range of the prepared concentration is determined by statistical process control of our production and analysis systems with a 95% confidence.

Cerilliant certifies that this standard meets or exceeds the specifications stated in this data sheet. Accuracy is ensured by purity determinations and gravimetric preparation using balances calibrated with NIST traceable weights. Precision is guaranteed by triplicate analysis and comparison to previous lots (when available). Homogeneity is demonstrated by random analysis of the ampuled standard.

Authorized Signature:

  
Lara Sparks, Quality Assurance Director

January 23, 2009

Date

*Standard Solution Comparability*

Standard Solution	Lot Number	Concentration <sup>3</sup> (mg/dL)	% Difference from Target
New Lot	FN020108-01	152.8	1.9
Previous Lot	FN101206-01	153.3	2.2

*Standard Solution Homogeneity*

Ampuling Position	Concentration <sup>3</sup> (mg/dL)	Mean	% RSD
Early	152.8	152.8	0.0
Middle	152.9		
Late	152.8		

<sup>3</sup> Concentration values are determined by comparison to an independent calibration curve prepared from a NIST standard (SRM 2897). We suggest using the prepared concentration value for dilutions. The concentration range is calculated from the distribution of multiple analyses of the new standard with a 95% degree of confidence.

*Standard Solution Assay Parameters*

Analysis Method: GC/FID Headspace  
 Column: DB-ALC1 30 m x 0.53 mm ID, 3.0 µm film thickness  
 Temp Program: 40°C hold for 12 min  
 Injector Temp: 200°C  
 Detector Temp: 250°C

Calibration Curve: Linear Regression  
 Number of Points: 4  
 Linearity (r): 0.999

*Each point is analyzed in triplicate.*


*Neat Material Data*

Compound Name: Ethanol  
 Compound Lot: 35330-42B  
 Chromatographic Purity: 99%

Chemical Formula: C<sub>2</sub>H<sub>6</sub>O  
 CAS Number: 64-17-5  
 Molecular Weight: 46.07

*Neat Material Verification*

**GC/FID Headspace Analysis**

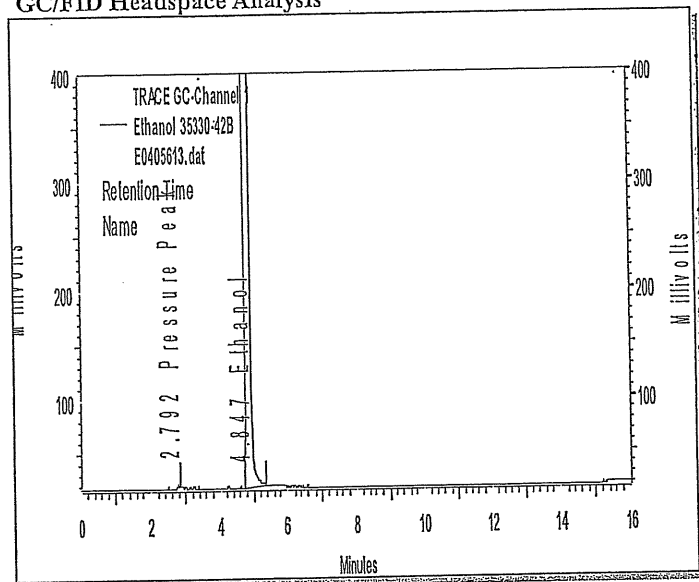

Column: DB-ALC1 30 m x 0.53 mm, 3 µm film thickness  
 Temp Program: 40°C (12 min) to 220°C at 40°C/min (5.5 min)  
 Carrier Gas: Helium  
 Flow Rate: 2.0 mL/min  
 Detector Temp: 250°C  
 Injector: Headspace Sampler  
 Injector Temp: 200°C  
 HS Oven Temp: 200°C  
 Injection Volume: 1.0 mL  
 Incubation Time: 10 minutes

Data File Name: C:\ChromQuest30\Projects\Default\Data\E0405613.dat  
 Operator: CAW  
 Instrument: GC#4  
 Method: AM1087  
 Sample Name: 35330-42B  
 Acquired: April 6, 2006 10:37 AM

Peak	Compound	Area	Area %
1	Pressure peak	NA	NA
2	Ethanol	322644078	100.0
Total			100.0



E-032  
 FN070209-01  
 Revision 0  
 Page 1 of 2

*Certificate of Analysis*  
*Certified Reference Standard - NIST Traceable*  
**Ethanol-200**  
*Ethyl Alcohol*

ISO GUIDE 34  
 CERTIFICATE ARI 353

ISO/IEC 17025  
 CERTIFICATE ARI 352

ISO 9001:2000  
 CERTIFICATE 3854

Catalog Number: E-032  
 Solution Lot: FN070209-01  
 Expiration Date: July 2014  
 Diluent: Water  
 Volume per Ampoule: 1.2 mL  
 Storage: Refrigerate. Do not freeze.  
 Intended Use: For laboratory use only. Not suitable for human or animal consumption.

- Expiration Date has been established through real time stability studies and applies to the ampoule stored unopened at the recommended storage condition.
- Ampoules are overfilled to ensure a minimum 1.2 mL volume fill. We advise laboratories to use measured volumes of this standard solution before diluting to the desired concentration. The standard should be used immediately after opening to avoid concentration changes due to evaporation.

Component	Solution Chromatographic Purity	Certified Concentration
Ethanol	100%	200.0 ± 0.7 mg/dL
<ul style="list-style-type: none"> <li>Uncertainty of the concentration, expressed in terms of volume, is an expanded uncertainty in accordance with ISO 17025 and ISO Guide 34 at the 95% confidence interval using a coverage factor of <math>k=2</math> and has been calculated by statistical analysis of our production methods applicable to ethanol reference standards and incorporates uncertainty of the purity factor, material density and mass measurement. The dispensing process is sufficiently controlled as to not be a significant contributor to uncertainty calculations and is, therefore, excluded. Solution stability is established through real time stability studies and is, therefore, excluded.</li> <li>When expressed in percentage terms, the relative standard uncertainty of the concentration is 0.175% and the relative expanded uncertainty is 0.35% at the 95% confidence interval (<math>k=2</math>).</li> <li>The purity factor (PF) mass balance measurement equation is used to calculate the amount of ethanol required to achieve an accurate concentration of the solution standard, accounting for both purity and residual water content.</li> <li>Purity factor has been established through independent certification of the neat analyte to ISO 17025 standards – See page 2.</li> <li>Solution purity is verified post ampouling and demonstrates no contamination or degradation has occurred.</li> </ul>		

**Traceability to SI through NIST:**

- This standard has been prepared and certified under the ISO Guide 34 and ISO/IEC 17025 standards and meets the requirements of a Certified Reference Material as defined by ISO.
- Gravimetrically prepared using qualified balances calibrated semi-annually by Mettler Toledo to ISO 17025 requirements and using NIST traceable weights. Qualification of each balance includes the assignment of a minimum weighing by Mettler Toledo taking into consideration the balance and installed environmental conditions to ensure each weighing complies with USP tolerances of NMT 0.1% relative uncertainty.
- Balance calibration adjustments are performed weekly utilizing the balance's internal adjustment mechanism and with NIST traceable weights.
- Balance calibration is verified prior to each use and is performed utilizing NIST traceable weights. Weigh tapes from the balance calibration are included in the production batch record for this standard. Production data package available upon request.
- Fill volume is gravimetrically verified throughout the dispensing process using qualified balances calibrated with NIST traceable weights.
- Weight sets used for all balance calibrations are calibrated externally by an ISO 17025 accredited calibration laboratory to NIST standards.
- Concentration of this standard has been analytically verified against a NIST SRM and a Control using a validated method. See page 2.

Cerilliant certifies that this standard meets the specifications stated in this certificate and warrants this product to meet the stated acceptance criteria through the expiration date. Warranty applies to ampoules stored unopened and stored under the recommended storage conditions. Warranty and expiry do not extend to solutions into which this product has been incorporated. Establishment of shelf life of all such products is the responsibility of the user.



*Lara Sparks*

Lara Sparks, Quality Assurance Director

*August 11, 2009*

Date




*Analytical Verification of Solution Standard Concentration and Batch Homogeneity:*

Solution Standard	Lot Number	Results compared to NIST SRM Lot 2895 (mg/dL)	Results compared to Control	Homogeneity (ampoule to ampoule consistency) % RSD
New Lot	FN070209-01	201.9	-0.11%	0.73%
Prior Lot	FN110107-02	201.3	-0.39%	1.53%
Acceptance Criteria		±2%	±2%	≤2%

▪ Concentration is calculated as the average of multiple analyses conducted using a validated Headspace GC/FID method. The validated GC/HS method has been demonstrated to adequately detect and quantitate ethanol concentrations ranging from 5 to 600 mg/dL. Relative standard uncertainty of the analysis is 1.675% and includes both uncertainty of the analytical method and uncertainty of the NIST SRM concentration.  
 ▪ The Control is independently prepared from a different lot of neat ethanol to ensure no bias in the analysis and independently qualified against a NIST SRM.  
 ▪ Homogeneity is ensured through rigorous production process controls statistically analyzed to evaluate risk and verified by analysis. The %RSD of samples pulled from across the lot using a stratified random sampling plan demonstrates ampoule to ampoule consistency or homogeneity of the New Lot.  
 ▪ The %RSD of the Prior Lot represents system suitability on the date of analysis. Triplicate injections of the Prior Lot are bracketed at the beginning and end of the sequence. %RSD criteria ensures proper system performance throughout the sequence.  
 ▪ All instruments used for certification of the neat materials and verification of the solution concentration and homogeneity are fully qualified through an Installation Qualification and an Operational Qualification which is repeated annually. System suitability is performed daily with rigorous acceptance criteria to ensure the system continues to perform within the validated parameters.

**Solution Standard Assay Parameters**


Analysis Method: GC/FID Headspace  
 Column: DB-ALCI 30 m x 0.53 mm ID, 3.0 µm film thickness  
 Temp Program: 40°C hold for 12 min  
 Injector Temp: 200°C  
 Detector Temp: 250°C

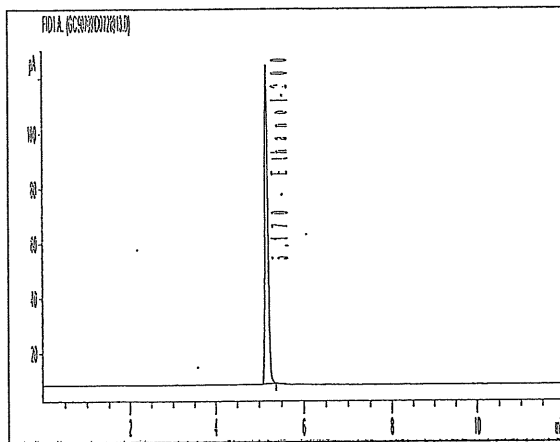

**Neat Material Analysis**


Purity by GC/FID Analysis: 100.00%  
 Water Content by Karl Fischer: 0.08%  
 Purity Factor: 99.92%

The purity factor (PF) mass balance measurement equation is used to calculate the amount of ethanol required to achieve an accurate concentration of the solution standard, accounting for both purity and residual water content.

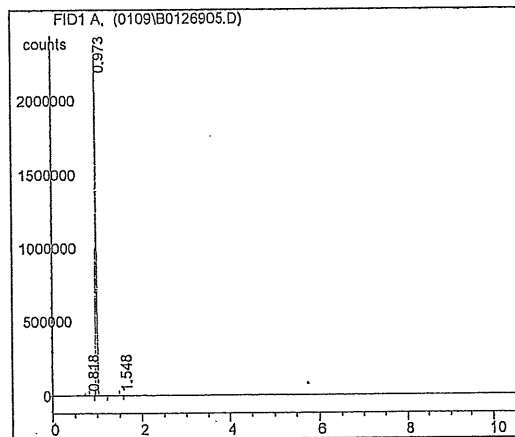



*Certificate of Analysis*  
*Certified Reference Material - NIST Traceable*  
**Ethanol-400**  
*Ethyl Alcohol*



**Catalog Number:** E-036  
**Solution Lot:** FN040909-01  
**Expiration Date:** April 2014  
**Diluent:** Water  
**Volume per Ampule:** 1.2 mL  
**Storage:** Protect from light, refrigerate. Do not freeze.  
**Intended Use:** For laboratory use only. Not suitable for human or animal consumption.

- Expiration Date has been established through real time stability studies.
- Ampules are overfilled to ensure a minimum 1.2 mL volume fill. We advise laboratories to use measured volumes of this solution standard before diluting to the desired concentration.

Component	Chromatographic Purity	Concentration
Ethanol	100%	400.0 ± 1.4 mg/dL
<ul style="list-style-type: none"> <li>Chromatographic purity of the solution is verified post ampuling to provide assurance of no contamination or degradation during manufacturing.</li> <li>Uncertainty of the concentration is expressed as an expanded uncertainty in accordance with ISO/IEC 17025 and ISO Guide 34 at the 95% confidence interval using a coverage factor of <math>k=2</math> and has been calculated by statistical analysis of our production system. Uncertainty includes uncertainty of the purity factor, material density and mass. Purity factor uncertainty incorporates uncertainty of all analyses performed to characterize the raw material including chromatographic purity and residual water. Mass uncertainty incorporates uncertainty of the balance in its installed environment and weighing technique and was determined through repeatability experiments using Cerilliant established weighing procedures.</li> <li>This standard meets the definition of a Certified Reference Material in accordance with ISO Guide 34.</li> </ul>		

**Traceability**

- This standard and its preparation are fully traceable to the SI through NIST.
- This standard was gravimetrically prepared using qualified balances calibrated semi-annually by Mettler Toledo, an ISO/IEC 17025 accredited company, using NIST traceable weights. Calibration verification is performed weekly through the range of the balance and then prior to each use. All calibration verifications are performed utilizing NIST traceable weights which are externally calibrated on an annual basis by a qualified ISO 17025 accredited calibration laboratory. Weigh tapes verifying pre-use balance calibration are included in the production batch record for this standard. Each balance has been assigned a minimum weighing by Mettler Toledo taking into consideration the balance and installed environmental conditions to ensure weighing complies with USP tolerances of no more than 0.1% relative error.
- Concentration is analytically verified by multiple analyses directly to a NIST SRM.

*Cerilliant certifies that this standard meets the specifications stated in this certificate and warrants this product to meet the stated acceptance criteria through the expiration date when stored unopened as recommended. Product should be used shortly after opening to avoid concentration changes due to evaporation. Warranty does not apply to ampoules stored after opening.*



*Lara Sparks*


Lara Sparks, Quality Assurance Director

*May 22, 2009*  
 Date

Analytical Verification of Solution Standard Concentration and Homogeneity					
Solution Standard	Lot Number	Concentration (mg/dL)	NIST SRM Lot and Concentration used for Assay	%RSD	
New Lot	FN040909-01	405.0	SRM 2896	1.7%	Homogeneity
Prior Lot	FN092507-01	397.7	0.2980% ± 0.0030%	0.9%	System Suitability

- Concentration is calculated as the average of multiple analyses by GC Headspace compared directly to the NIST SRM lot listed above. Acceptance criteria of ± 2.0% incorporates variability of the analysis. Concentration of the NIST SRM lot is as certified by NIST.
- Homogeneity of the New Lot is ensured through the use of validated processes and verified by analysis. The %RSD of samples pulled from across the lot demonstrates homogeneity of the New Lot.
- The %RSD of the Prior Lot represents variability of the analysis performed during solution standard release testing and system suitability. Triplicate injections of the Prior Lot are bracketed at the beginning and end of the sequence. %RSD criteria of ≤ 2% ensures system performance throughout the sequence.
- All testing equipment is fully qualified through an installation qualification and annual operational qualifications.

Solution Standard Assay Parameters	
Analysis Method:	GC/FID Headspace
Column:	DB-ALC1 30 m x 0.53 mm ID, 3.0 µm film thickness
Temp Program:	40°C hold for 12 min
Injector Temp:	200°C
Detector Temp:	250°C

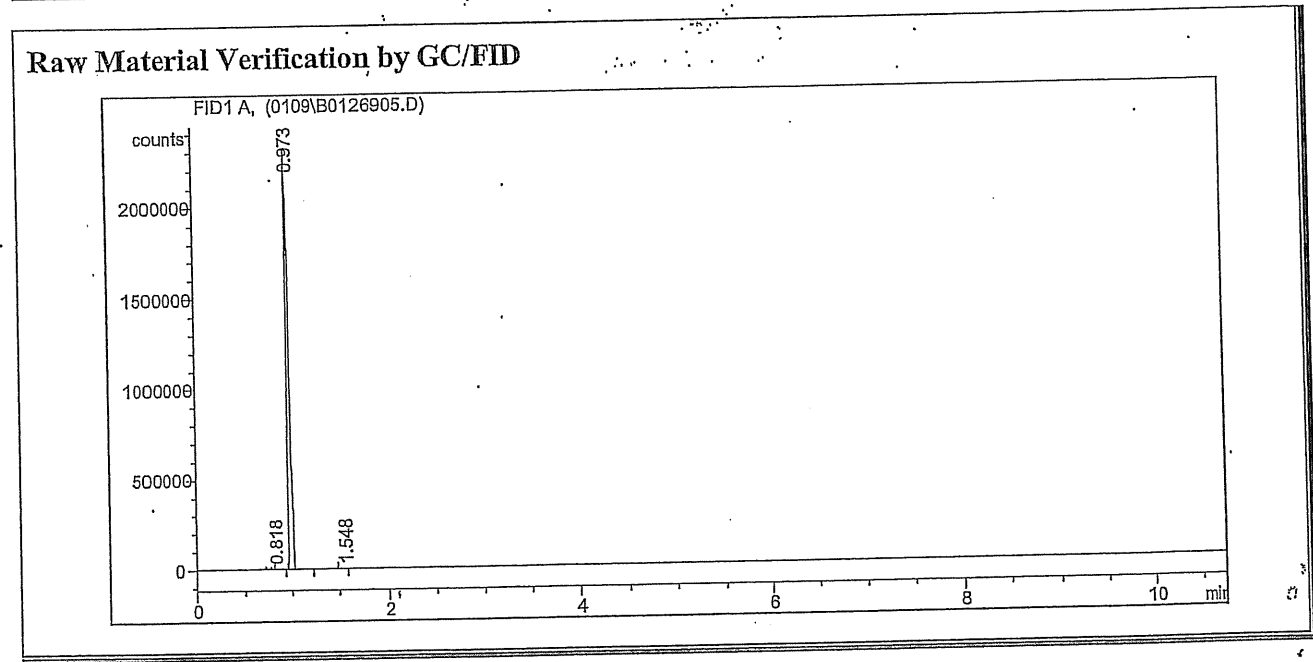





E-053  
FN011408-01  
Revision 1


# Certificate of Analysis

ISO GUIDE 34  
ACCREDITED  
CERTIFICATE ARI353  
ISO/IEC 17025  
ACCREDITED  
CERTIFICATE ARI352  
ISO 9001:2000  
CERTIFIED  
CERTIFICATE 2054

## Ethanol-500

*Ethyl alcohol*

Catalog Number: E-053  
Solution Lot: FN011408-01  
Expiration Date: January 2013  
Solvent: Water  
Amount per Ampule: 1.2 mL  
Storage: Protect from light, refrigerate. Do Not Freeze.  
Handling: We advise laboratories to use measured volumes of this standard solution before diluting to the desired concentration.  
Intended Use: For laboratory use only. Not suitable for human or animal consumption.



Component	Chromatographic Purity <sup>1</sup>	Concentration <sup>2</sup>
Ethanol	99%	500.0 ± 15.5 mg/dL

<sup>1</sup> Determined by chromatographic analysis. See following pages for more information.

<sup>2</sup> The range of the prepared concentration is determined by statistical process control of our production and analysis systems with a 95% confidence.

Cerilliant certifies that this standard meets or exceeds the specifications stated in this data sheet. Accuracy is ensured by purity determinations and gravimetric preparation using balances calibrated with NIST traceable weights. Precision is guaranteed by triplicate analysis and comparison to previous lots (when available). Homogeneity is demonstrated by random analysis of the ampuled standard.

Authorized Signature:

  
Lara Sparks, Quality Assurance Director

January 23, 2009

Date

**Standard Solution Comparability**

Standard Solution	Lot Number	Concentration <sup>3</sup> (mg/dL)	% Difference from Target
New Lot	FN011408-01	506.7	1.3
Previous Lot	FN071406-01	505.5	1.1

**Standard Solution Homogeneity**

Ampuling Position	Concentration <sup>3</sup> (mg/dL)	Mean	% RSD
Early	505.8		
Middle	504.5		
Late	509.8	506.7	0.5

<sup>3</sup> Concentration values are determined by comparison to an independent calibration curve prepared from a NIST ethanol standard (SRM 2897). We suggest using the prepared concentration value for dilutions. The concentration range is calculated from the distribution of multiple analyses of the new standard with a 95% degree of confidence.

**Standard Solution Assay Parameters**


Analysis Method:	GC/FID Headspace	Calibration Curve:	Linear Regression
Column:	DB-ALC1 30 m x 0.53 mm ID, 3.0 µm film thickness	Number of Points:	4
Temp Program:	40°C hold for 12 min	Linearity (r):	0.999
Injector Temp:	200°C		
Detector Temp:	250°C		

**Neat Material Data**

Compound Name:	Ethanol	Chemical Formula:	C <sub>2</sub> H <sub>6</sub> O
Compound Lot:	35330-42B	CAS Number:	64-17-5
Chemical Purity:	99%	Molecular Weight:	46.07

**Spectral and Physical Data**

**GC/FID Headspace Analysis**

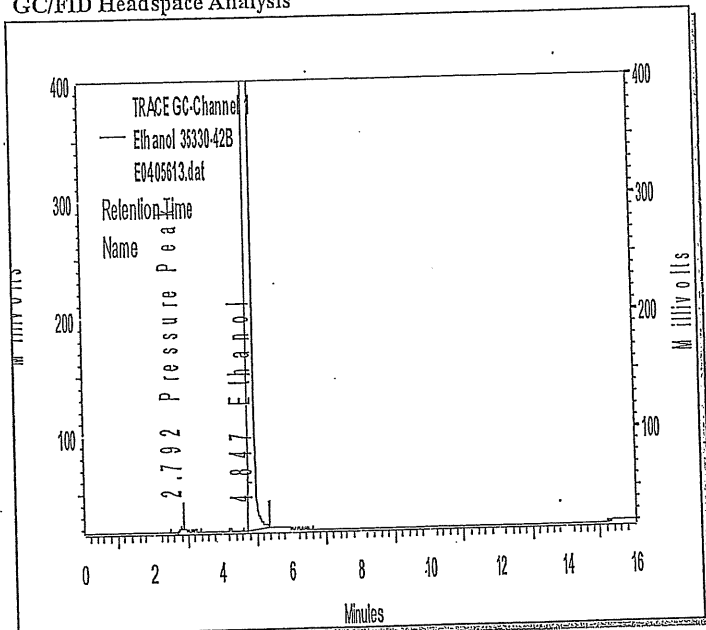

Column:	DB-ALC1 30 m x 0.53 mm, 3 µm film thickness
Temp Program:	40°C (12 min) to 220°C at 40°C/min (5.5 min)
Carrier Gas:	Helium
Flow Rate:	2.0 mL/min
Detector Temp:	250°C
Injector:	Headspace Sampler
Injector Temp:	200°C
HS Oven Temp:	200°C
Injection Volume:	1.0 mL
Incubation Time:	10 minutes

Data File Name:	C:\ChromQuest30\Projects\Default\Data\E0405613.dat
Operator:	CAW
Instrument:	GC#4
Method:	AM1087
Sample Name:	35330-42B
Acquired:	April 6, 2006 10:37 AM

Peak	Compound	Area	Area %
1	Pressure peak	NA	NA
2	Ethanol	322644078	100.0
Total			100.0



110 Benner Circle  
 Bellefonte, PA 16823-8812  
 Tel: (800)356-1688  
 Fax: (814)353-1309

www.Restek.com



## Certificate of Analysis

**FOR LABORATORY USE ONLY-READ MSDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 36237 **Lot No.:** A086511  
**Description :** 0.15 g/dL Ethanol Standard  
Forensic Ethanol Solution 0.15g/dL, Water, 1mL/ampul 5pk  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** June 2016 **Storage:** 10°C or colder

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)		
1	Ethanol (BAC) CAS # 64-17-5 Purity 99%	0.150 g/dL	+/- 0.000874	g/dL	Gravimetric
			+/- 0.003320	g/dL	Unstressed
			+/- 0.003333	g/dL	Stressed
<b>Solvent:</b>	Water CAS # 7732-18-5 Purity 99%				

**Specific Reference Material Notes:**

This standard is NIST traceable in two ways:

1. The ethanol that was used in this standard was weighed out on an analytical balance that is calibrated daily with NIST traceable weights. The weights that are used for this calibration are recertified yearly by Troemner, Inc. Troemner, Inc. compares our weight set to reference mass standards that are directly traceable to the NIST under test number 822/264157-00.
2. This standard was tested versus an NIST ethanol standard. The NIST ethanol standard was used to make a 3 point calibration curve. The Restek Corporation manufactured ethanol standard and the NIST calibration standards were analyzed using GC/FID. The concentration of the Restek ethanol standard was calculated using the 3 point NIST calibration curve.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.Restek.com

## Certificate of Analysis

FOR LABORATORY USE ONLY-READ MSDS PRIOR TO USE.

**Catalog No. :** 36266 **Lot No.:** A084662  
**Description :** 0.4 g/dL Forensic Ethanol Standard  
Blood Alcohol Mix 0.4g/dl forensic ethanol solution, H2O, 1ml/ampule, 5pk  
**Container Size :** <sup>5</sup>2 mL **Pkg Amt:** <sup>5</sup>> 1 mL  
**Expiration Date :** <sup>1</sup>February 2016 **Storage:** 10°C or colder

Elution Order	Compound	CAS #	Percent Purity <sup>2</sup>	Grav. Conc. (weight/volume) <sup>3</sup>	Grav.Uncert. (95% C.L.; K=2) <sup>4</sup>
1	Ethanol (BAC)	64-17-5	99%	0.400 g/dL	+/- 0.002326 g/dL
<b>Solvent:</b>	Water	7732-18-5	99%		

**Column:**  
30m x .32mm x 1.2um  
BAC2 (cat.#18002)


**Carrier Gas:**  
hydrogen @ head pressure 7 psi

**Temp. Program:**  
40°C (hold 6 min.)

**Inj. Temp:**  
250°C

**Det. Temp:**  
270°C

**Det. Type:**  
FID

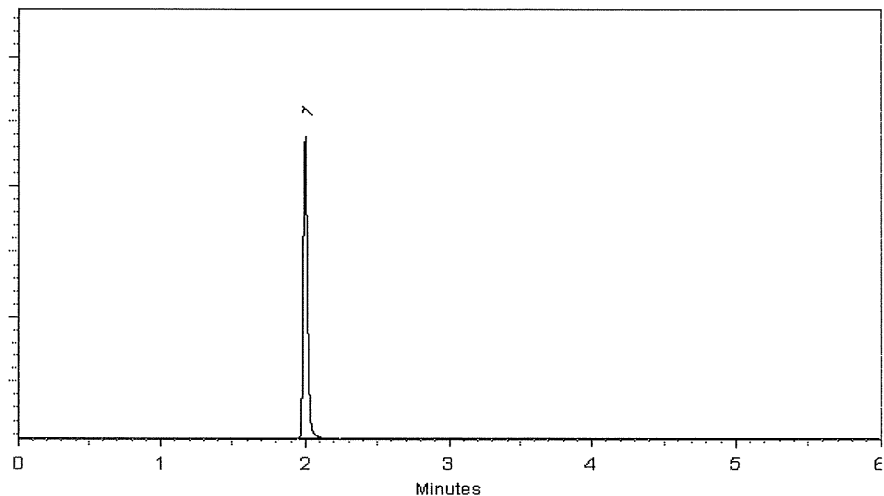

*Christopher Zucco*  
Christopher Zucco - QA Analyst

Date Passed: 21-Oct-2011 Balance: 1127510105

Manufactured under Restek's ISO 9001:2008  
Registered Quality System  
Certificate #FM 80397

- 1 Expiration date of the unopened ampule stored at the recommended storage condition is the last day of the month listed.
- 2A Purity and chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ECD, GC/MS. Purity value is rounded to the nearest whole number. See data pack or contact Restek for further details.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities.
- 2C The following types of compounds will have a listed purity of less than 99%: Aldehyde/Ketone-DNPH compounds, Bromides, Chlorides, HCL salts, HBR salts, sulfates, hydrates, and other compounds as necessary. The listed purity is a correction factor that is equivalent to the percentage of parent compound in the molecule. This correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution. The concentration listed on the certificate is the concentration of the parent compound in the solution.
- 2D Purity of isomeric compounds is reported as the sum of the isomers. Value is rounded to the nearest whole number after summation.
- 3 Based upon gravimetric preparation with balance calibration verified using NIST traceable weights (seven mass levels) and/or class A glassware used for dilutions.
- 4 Uncertainties determined using data for balances and glassware from measurement systems analysis methodology, raw material purity, and, when significant, equipment tolerances or calibration results.
- 5A Containers are overfilled to ensure the packaged amount, as a minimum.
- 5B Restek supplies deactivated vials along with most standards packed in 2 mL ampules, for the handling and storage of standards. Due to space constraints, Restek does not supply vials for larger volume ampules. Samples should be transferred into deactivated vials for handling and storage. Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31840, which includes complete instructions. Restek will also deactivate larger volume vials from our inventory, as a custom ordered item. Contact your Restek sales or customer service representative for details.

Note:

This standard is NIST traceable in three ways:

1. The ethanol that was used in this standard was analyzed by Restek Corporation using GC/mass spec. The mass spectra that was generated was compared to the ethanol spectra in the NIST mass spectra library to ensure an exact match. This spectral data is included in this data package.
2. The ethanol that was used in this standard was weighed out on an analytical balance that is calibrated daily with NIST traceable weights. The weights that are used for this calibration are recertified yearly by Troemner, Inc. Troemner, Inc. compares our weight set to reference mass standards that are directly traceable to the NIST under test number 822/264157-00.
3. This standard was tested versus an NIST ethanol standard. The NIST ethanol standard was used to make a 3 point calibration curve. The Restek oration manufactured ethanol standard and the NIST calibration standards were analyzed using GC/FID. The concentration of the Restek ethanol standard calculated using the 3 point NIST calibration curve.